

We are IntechOpen, the world's leading publisher of Open Access books Built by scientists, for scientists

5,200

Open access books available

128,000

International authors and editors

150M

Downloads

Our authors are among the

154

Countries delivered to

TOP 1%

most cited scientists

12.2%

Contributors from top 500 universities



WEB OF SCIENCE™

Selection of our books indexed in the Book Citation Index
in Web of Science™ Core Collection (BKCI)

Interested in publishing with us?
Contact book.department@intechopen.com

Numbers displayed above are based on latest data collected.
For more information visit www.intechopen.com



Multisyringe Flow Injection Analysis for Environmental Monitoring: Applications and Recent Trends

Marcela A. Segundo¹, M. Inês G. S. Almeida^{1,2} and Hugo M. Oliveira¹

¹REQUIMTE, Department of Chemistry, Faculty of Pharmacy, University of Porto,

²School of Chemistry, University of Melbourne,

¹Portugal

²Australia

1. Introduction

Multisyringe flow injection analysis (MSFIA) was introduced by Víctor Cerdà and co-workers in 1999 (Cerdà et al., 1999) as a robust alternative to its predecessor flow injection techniques, combining the multi-channel operation of flow injection analysis (Ruzicka & Hansen, 1975) with the possibility of flow reversal and selection of the exact volume of sample and reagent required for analysis as presented in sequential injection analysis (Ruzicka & Marshall, 1990). Generally, flow injection systems are automation tools where, in opposition to batch conventional assays, physico-chemical equilibrium is not attained prior to determination. Hence, flow injection analysis is based in three principles: (1) reproducible sample injection or insertion in a flowing carrier stream; (2) controlled dispersion of the sample zone; and (3) reproducible timing of its movement from the injector point to the detection system.

Since its inception, MSFIA has been the basis for automation of more than 120 different assays, reviewed in several publications (Almeida et al., 2011; Magalhães et al., 2009; Maya et al., 2009; Segundo & Magalhães, 2006). This type of automatic flow injection systems is based on the utilization of a multisyringe burette, depicted schematically in Fig. 1A and 1B. It is a multiple channel piston pump, containing up to four syringes, driven by a single motor of a usual automatic burette and controlled by computer software through a serial port. A two-way commutation valve is connected to the head of each syringe, allowing optional coupling to the manifold lines or to the solution reservoir.

Because the four syringes are driven by the same motor, all pistons move at once in the same direction either delivering (dispense operation) or loading the syringes (pickup operation) with liquids. Considering that the commutation valves can be placed in two positions, there are four possibilities for flow management as depicted in Fig. 1C. Hence, when the pistons are moving upwards, it is possible to dispense liquid into the flow system or send it back to its reservoir. This feature enables that only the necessary amount of reagent solution is introduced into the flow system. Furthermore, when the pistons are moving downwards, it is possible to refill the syringes with solutions present in the respective vessel or to aspirate solutions from the system in order to perform the sampling operation.

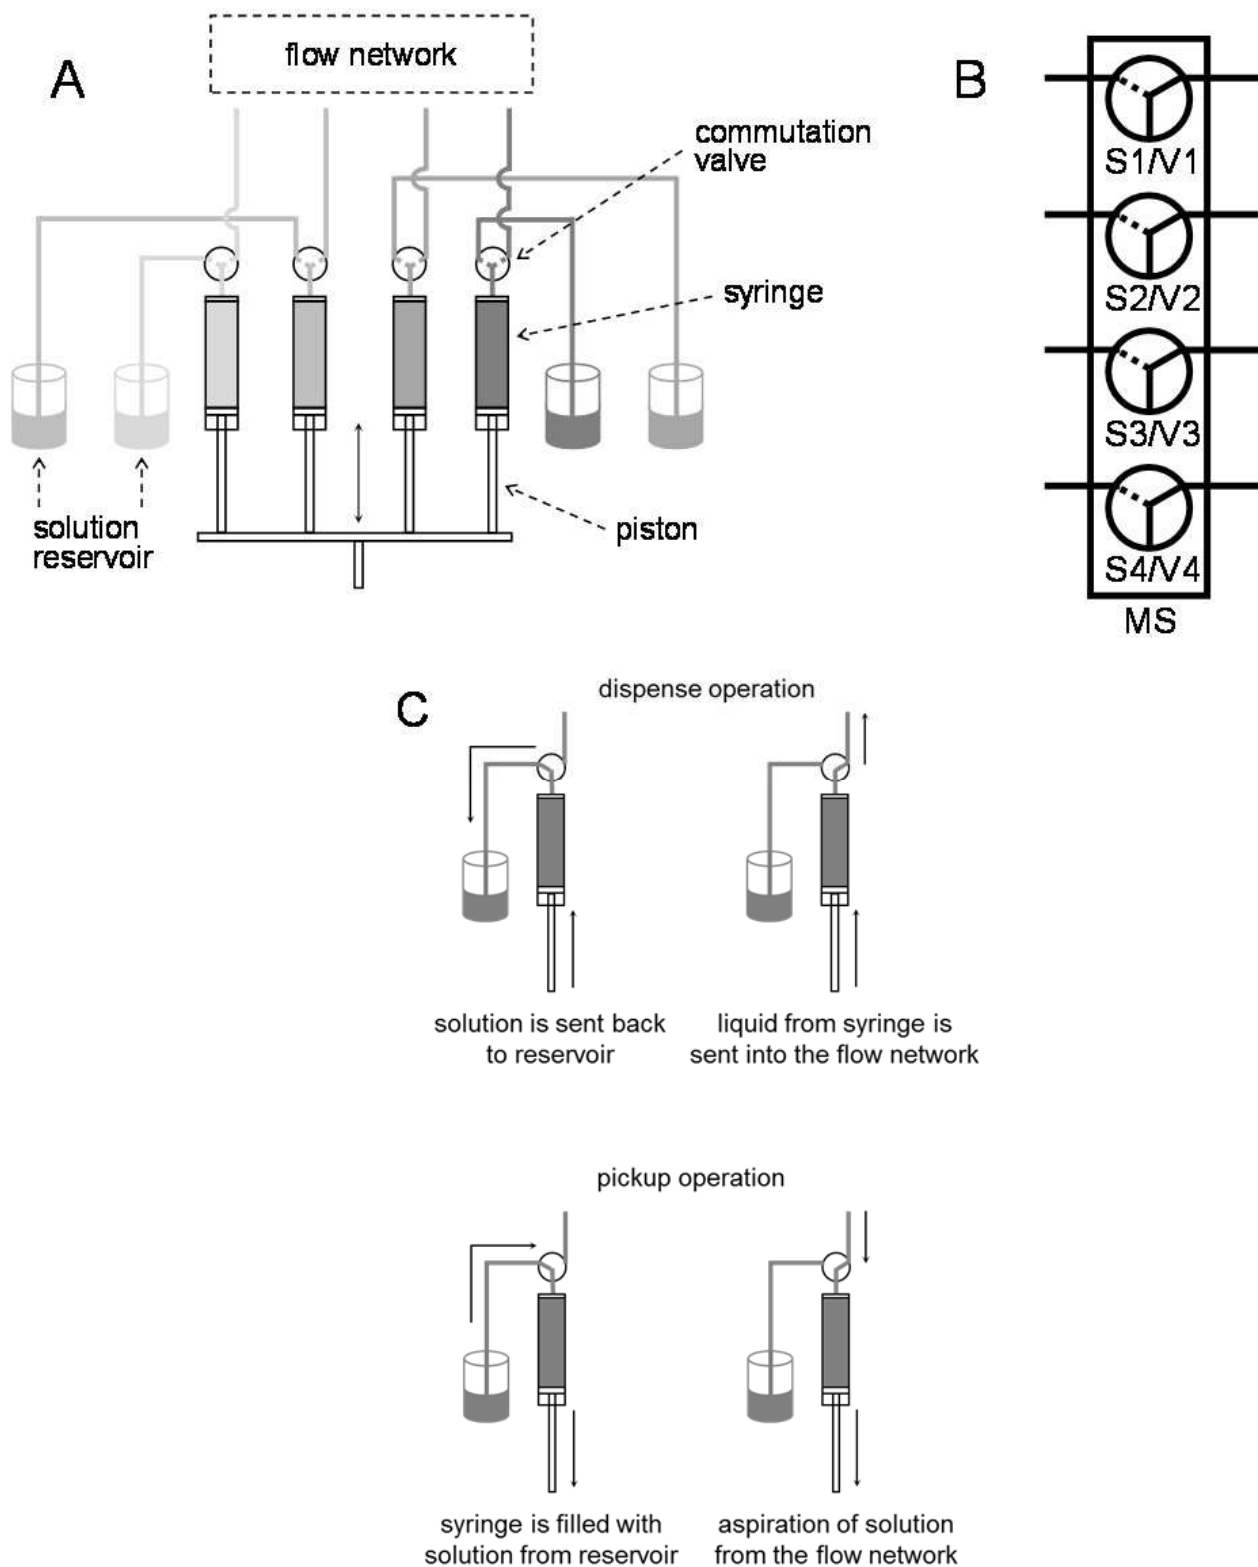


Fig. 1. Schematic representation of multisyringe apparatus, with indication of the different components (A) or simplified (B). Flow management possibilities for one syringe during operation of multisyringe apparatus are also given (C). MS = multisyringe; S = syringe, V = commutation valve.

Syringes with different volumes, ranging from 0.5 to 25 ml are available, enabling the application of a wide range of flow rates. For example, for a 5 ml syringe, flow rates ranging from 0.28 to 15 ml min⁻¹ may be attained (Miró et al., 2002). Nevertheless, once the flow rate (and volume) is fixed for one syringe, it is also defined for the other channels, and it will depend on the ratio between syringe capacities as different syringes can be placed in any of the four positions.

Finally, MSFIA manifolds are not restricted to the syringes and the respective commutation valves. The presence of four digital outputs, each capable of providing 12 V/0.5 A, allows the utilization of up to 12 additional commutation valves, also controlled through the multisyringe apparatus. These extra commutation valves are often necessary to assemble a flow network, where analyte determination and sample treatment can be implemented by including confluences for reagent addition, suitable detectors (spectrophotometers, fluorimeters, flame or atomic emission spectrometers) and devices for mass transfer (gas diffusion or dialysis units), for instance.

2. Applications of MSFIA to environmental monitoring

MSFIA systems have been successfully applied to the determination of more than 20 species in environmental samples as illustrated in Tables 1 and 2.

Several applications were targeted to plant macronutrients, such as potassium and phosphorus, and also to micronutrients, including boron, iron and selenium (Table 1). These species were quantified in different types of water (natural and seawater) and also in soil extracts or even soil slurries when applying flame emission spectrometry for determination of potassium (Almeida et al., 2008). The introduction of aqueous samples in flow systems is rather trivial, while manipulation of samples containing suspended solids is not common, requiring a special manifold design employing larger commutation valves and large bore tubing (Almeida et al., 2008).

In fact, solid environmental samples were successfully handled within MSFIA systems. Extraction of potassium contained in 1.8 g of soil was performed in-line, prior to potentiometric determination. The soil was placed in a container where 9 ml of Morgan extractant solution was delivered automatically by one of the syringes. After 6 min, in-line filtration took place, and a small portion of filtrate (100 µl) was sent to the potentiometric detector after in-line addition of an ionic strength adjusting buffer. Different soils were analyzed consecutively without carry-over effects and the filtration unit was reutilized up to 10 times (Almeida et al., 2006).

Besides the determination of total extractable content, MSFIA systems have been employed to dynamic fractionation testing schemes, profiting from its inherent capabilities of controllable flow programming. In fact, Miró and co-workers developed a multiple stirred-flow chamber assembly, containing up to three parallel extractors, to perform sequential extraction of readily mobilizable fractions of trace elements (Cu, Cd, Ni, Pb, Zn) in fly ashes (Boonjob et al., 2008). Though the detection step was performed off-line (not automated) on each 10 ml fraction collected, the MSFIA system still provided information about overall extractable pools in less than 2 hours, a drastic reduction of time when compared to 18 to 24 hours required per fraction in equilibrium leaching tests. Moreover, the implementation of a sequential leaching scheme was easily accommodated in MSFIA, due to its inherent flow features and also by housing different extracting solutions (water, 0.11 M acetic acid, 0.11 M acetic acid/acetate buffer) simultaneously in each syringe of the multisyringe burette.

Analyzed species	Sample type	In-line sample treatment	Determination throughput (h ⁻¹)	Reference
Boron (available)	Soil extract	---	15	(Gomes et al., 2005)
Iron (available)	Soil extract	---	34	(Gomes et al., 2005)
Iron (total)	Water	Solid phase extraction	12	(Pascoa et al., 2009)
Iron (total) and Fe(III)	Water	---	60	(Pons et al., 2004)
Iron (total) and Fe(III)	Water (natural and seawater)	Solid phase extraction	5 - 10	(Pons et al., 2004, 2005a, 2005b)
Phosphate	Water	Solid phase extraction	11	(Morais et al., 2004)
Phosphate	Soil extract	In-line sequential extraction	Not given	(Buanuam et al., 2007)
Phosphorus (available)	Soil extract	---	15	(Almeida et al., 2005)
Phosphorus	Water	Microwave digestion	12	(Almeida et al., 2004)
Potassium	Soil extracts	Extraction and in-line filtration	13	(Almeida et al., 2006)
Potassium	Soil slurries	---	28	(Almeida et al., 2008)
Selenium	Sea lettuce	---	84	(Semenova et al., 2003)
Selenium	Water (natural and seawater)	Solid phase extraction	8	(Serra et al., 2010)

Table 1. MSFIA methods for nutrient assessment and monitoring

The same group proposed a fully automated strategy for fractionation of orthophosphate in soil samples and in-line spectrophotometric determination resorting to molybdenum blue reaction (Buanuam et al., 2007). The system integrated dynamic sequential extraction using 1 M ammonium chloride solution, 0.1 M sodium hydroxide solution and 0.5 M hydrochloric acid solution as extractants according to the Hieltjes-Lijklema scheme. Solid soil samples were placed in a flow-through customized dual conical chamber (Chomchoei et al., 2004), which could be filled with up to 300 mg of soil. Compared to conventional batch equilibrium procedures, the automatic dynamic fractionation system offered further knowledge on: (i) the extraction kinetics, (ii) the content of phosphorus in available pools, (iii) the efficiency of the leachants and (iv) the actual extractant volume required for quantitative release of orthophosphate. The automatic MSFIA extraction scheme was also validated through application to certified reference material SRM 2704 river sediment and SRM 2711 Montana soil.

Recently, a similar strategy was applied for automated dynamic extraction and determination of readily bioaccessible chromium(VI) in soils. Besides the extraction capabilities, the automatic MSFIA system also fostered in-line quantification of Cr(VI)

after derivatization using 1,5-diphenylcarbazide and in-line adjustment of Cr(VI) concentration prior to determination. This last feature was attained by incorporating a dilution chamber (for extracts from highly contaminated samples) and another flow-through column filled with multi-walled carbon nanotubes for preconcentration of Cr-1,5-diphenylcarbazide (for extracts or fractions with low Cr(VI) concentration). The MSFIA system was successfully applied to SRM 2701 soil, providing the extraction kinetics for sequential extraction using water and an acid rain surrogate. The automatic integration of extraction and Cr(VI) determination also allowed the minimization of interconversion between Cr oxidation states often observed when determination is not carried out immediately after extraction.

In fact, several MSFIA systems were developed for monitoring of environmental pollutants as indicated in Table 2. Both organic and inorganic species were targeted, with a focus on water analysis. In this context, in-line sample treatment is undeniably a requisite when devising monitoring schemes with real environmental samples. There are two main reasons for this. First, analytes, particularly pollutants, are generally present at low concentrations (ppt or ppb range) in these samples, requiring a preconcentration step in order to meet the linear working range offered by the available detection systems. Secondly, the target analyte may be strongly bound or entrapped in the sample matrix or it can present different forms concerning its oxidation state. Hence, solid phase extraction has been frequently implemented in-line, aiming the enrichment and selective uptake of analytes. It has been applied for the determination of trace levels of phosphate ($5 - 50 \mu\text{g l}^{-1}$ of P) in natural waters combined to chemiluminescence detection (Morais et al., 2004), for determination of selenium ($5.7 - 1290 \mu\text{g l}^{-1}$) in natural and seawater (Serra et al., 2010) and for determination of trace iron ($0.05 - 8 \mu\text{g l}^{-1}$; $0.2 - 42 \mu\text{g l}^{-1}$) in waters (Pascoa et al., 2009; Pons et al., 2004, 2005a, 2005b) as far as nutrient analysis is concerned.

Solid phase extraction has also been employed in more than half of the applications focusing on pollutants monitoring and it was implemented in several ways. In flow injection systems, sorbents are generally packed in flow-through columns, which are sequentially percolated by conditioning solution, sample, washing solution and eluent, fostering selective retention of target analyte(s), followed by its/their elution after sample matrix removal. This strategy has also been implemented in MSFIA for determination of total phenolics in waters, using Amberlite XAD-4 as sorbent and in-line derivatization with 4-aminoantipyrine (Oliveira et al., 2005). This MSFIA system was further improved and coupled to liquid chromatography, allowing on-line preconcentration and determination of eleven priority phenolic pollutants in water and soil samples (Oliveira et al., 2009).

Extraction membranes, containing different functional groups, have also been employed in MSFIA systems as they are an advantageous alternative to particulate sorbents because they allow higher flow rates (providing high determination throughputs) and low backpressure, avoiding leakages and clogging. Several applications have been reported, namely for preconcentration of nitrophenols and their determination after elution (Manera et al., 2007a) or using optosensing (Manera et al., 2007b) by probing the extraction membrane with a bifurcated optical fiber connected to a CCD spectrometer. In fact, the utilization of optosensors in MSFIA systems is simplified because all solutions required (sample, conditioning and regenerating solutions) can be automatically delivered by the multisyringe burette in a precise and timely way. Hence, optosensing has also been applied in MSFIA systems for trace level determination of 1-naphthylamine in water samples (Guzmán-Mar et al., 2006b) and determination of sulphide (Ferrer et al., 2005b).

Analyzed species	Sample type	In-line sample treatment	Determination throughput (h ⁻¹)	Reference
Arsenic	Water, fish muscle and liver	---	108	(Semenova et al., 2002)
Arsenic	Water	Solid phase extraction	9	(Long et al., 2006)
Arsenic (total inorganic) and As(III)	Water, sea lettuce	---	10	(Leal et al., 2006b)
Azinphos methyl	Water	Hydrolysis	7	(Ornelas-Soto et al., 2009)
Chlorotriazine herbicides	Water and soil extracts	Solid phase extraction	Not given	(Boonjob et al., 2011; Boonjob et al., 2010)
Chromium(VI)	Soil leachates	In-line extraction	Not given	(Rosende et al., 2011)
Halogenated organic carbons	Water and leachates	Solid phase extraction	9	(Maya et al., 2008)
Mercury	Water, fish muscle	---	44	(Leal et al., 2006a)
Mercury	Water and leachates	Solid phase extraction	30	(Serra et al., 2008)
Mercury (inorganic and organic)	Water, fish muscle	Solid phase extraction	14	(Serra et al., 2009)
1-Naphthylamine	Water	---	90	(Guzmán-Mar et al., 2006a)
1-Naphthylamine	Water	Solid phase extraction	14	(Guzmán-Mar et al., 2006b)
Nitrophenols	Water, seawater and waste leachates	Solid phase extraction	3 - 11	(Horstkotte et al., 2008; Manera et al., 2007a; Manera et al., 2007b)
Nitrophenols	Water	Liquid-liquid extraction	11	(Miró et al., 2001)
Pharmaceutical residues (NSAIDs)	Water	Solid phase extraction	Not given	(Quintana et al., 2006)
Pharmaceutical residues (thiazide diuretics)	Water and solid waste leachates	Solid phase extraction	12	(Maya et al., 2010)
Phenolic compounds (total)	Water	Solid phase extraction	4 - 16	(Oliveira et al., 2005)
Phenolic compounds	Water and soil	Solid phase extraction	4 - 10	(Oliveira et al., 2009)
Polychlorinated biphenyls	Solid waste leachates	Solid phase extraction	Not given	(Quintana et al., 2009)
Sulphide	Water	---	45	(Ferrer et al., 2004)
Sulphide	Wastewater	Analyte separation by gas diffusion	13 - 20	(de Armas et al., 2004; Maya et al., 2007)
Sulphide	Waters (fresh, seawater and wastewater)	Solid phase extraction	5 - 8	(Ferrer et al., 2005a, 2005b; Ferrer et al., 2006)
Warfarin	Water	Solid phase extraction	12	(de Armas et al., 2002)
Sulphonated azo dyes	Water	---	7.5	(Fernandez et al., 2010)
UV filters	Water (seawater and swimming pool)	Solid phase extraction	7	(Oliveira et al., 2010)

Table 2. MSFIA methods for assessment and monitoring of pollutants

MSFIA systems were also devised for speciation of arsenic (Leal et al., 2006b) and mercury (Serra et al., 2009) in environmental samples. For arsenic, As(III) was quantified by atomic fluorescence spectrometry while As(V) was assessed by difference from total As content, determined for the same sample after in-line reduction of As(V) to As(III) by automatic addition of potassium iodide and ascorbic acid. For mercury, atomic fluorescence spectrometry was also employed and speciation between inorganic and organic (methylmercury) forms was performed by selectively retaining mercury tetrachloro complex in an anion exchange membrane, while organic mercury was directed towards a flow-through UV digester before detection. Inorganic mercury was later eluted from the membrane by in-line reduction with tin chloride, allowing a limit of detection of 16 ng l⁻¹.

Besides the reduction of intervention from laboratory technicians in the analytical operations, automation of environmental assays by MSFIA provided also an acceptable determination throughput, ranging from 7.5 to 108 determinations per hour in automatic systems where no sample treatment was required or where it was performed off-line. For MSFIA systems comprising in-line sample treatment, determination throughputs ranged from 3 to 30 determinations per hour, which are excellent figures. For instance, the determination of total phosphorus in waste water samples was carried out with a determination throughput of 12 determinations per hour by implementing in-line microwave digestion of samples (Almeida et al., 2004). This is a significant reduction of the assay time when compared to the conventional batch digestion that took about 2 hours for quantitative measurements.

3. Recent trends for sample treatment

As mentioned before, environmental samples comprise complex matrices where target analytes are not generally amenable to direct determination by instrumental analysis, requiring sample treatments. Regarding this aspect, solid phase extraction is undoubtedly the most common treatment applied in MSFIA systems as shown in Tables 1 and 2. Besides the examples presented before in the text, MSFIA capabilities have been recently exploited to perform solid phase extraction using bead injection (BI) prior to chromatographic analysis.

The bead injection concept consists of handling solid suspensions in a fully automatic fashion, where the solid-phase sorbent, presented as micrometric beads, is renewed in each individual analytical cycle, rendering a fresh portion of sorbent for each analysis. Moreover, bead injection allows the simultaneous monitoring of both effluent and solid phase itself (optosensing) in real time, which brings complementary and enhanced insight into the solid phase extraction procedure in a single assay (Gutzman et al., 2006).

The bead injection concept is often associated to the lab-on-valve (LOV) platform. The LOV module comprises a monolithic structure with microconduits machined in a polymethylmethacrylate or polyetherimide unit, which is mounted atop a multiposition valve (Fig. 2), representing a step forward towards automation and miniaturization of flow injection systems. The LOV-BI approach offers two main advantages, not matched by any other automatic, flow-based solid phase extraction scheme: (i) the automatic renewal of sorbent, without any intervention of operator or replacement of devices or physical parts of the system, so as to circumvent the progressive deactivation and tighter packing of permanent in-line solid phase extraction cartridges; and (ii) the accurate metering of sorbent and eluate quantities by resorting to bi-directional programmable flow, as precisely controlled by the multisyringe burette (Miró et al., 2011).

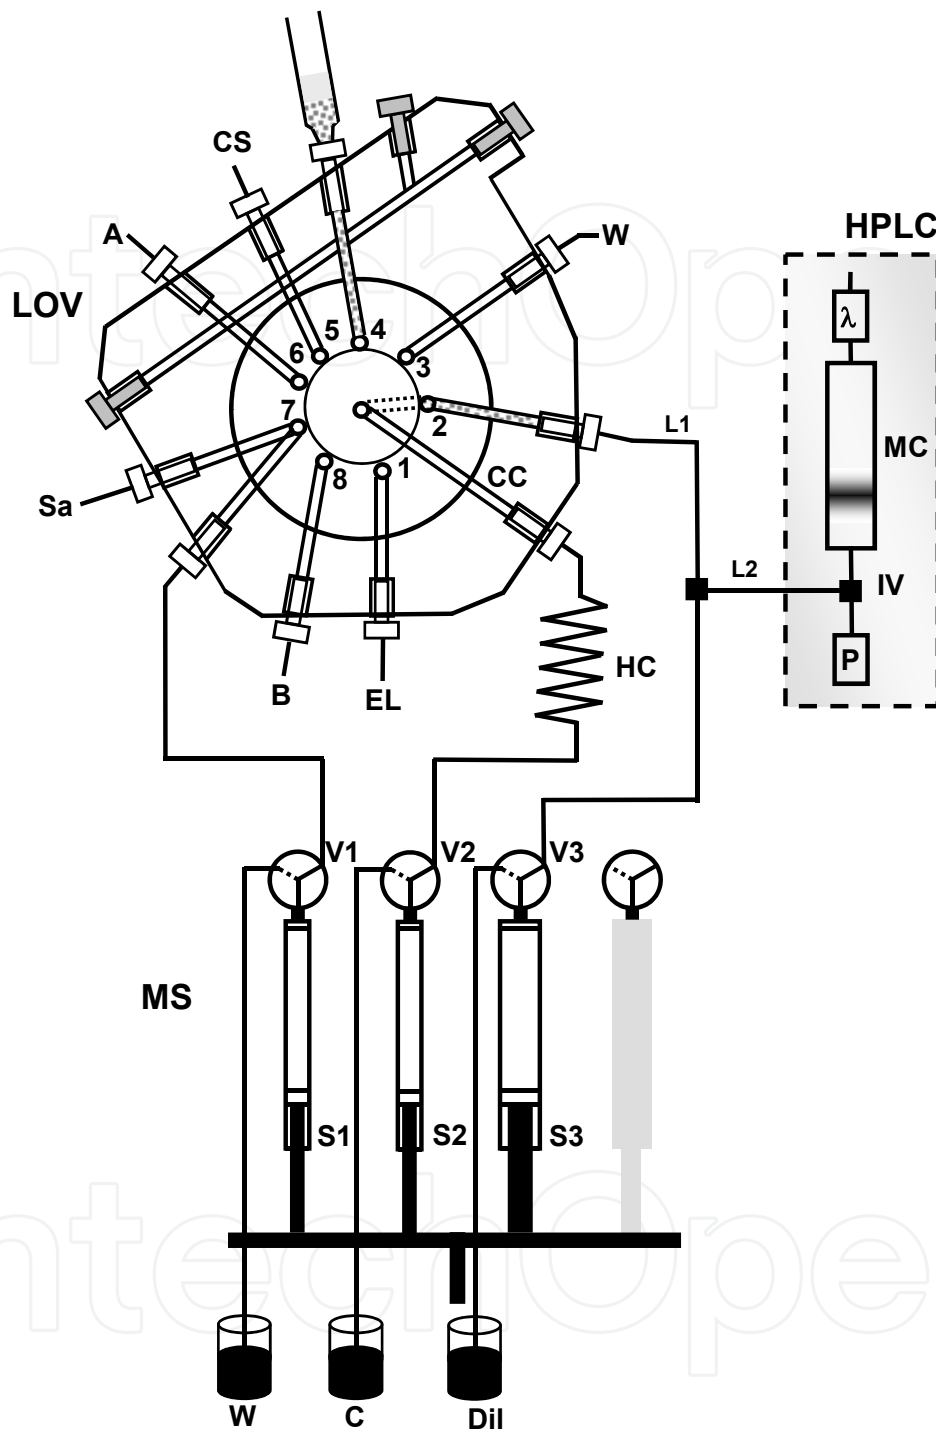


Fig. 2. Schematic representation of multisyringe flow injection system coupled to lab-on-valve for sample treatment, hyphenated to liquid chromatography. LOV: lab-on-valve, MS: multisyringe, HPLC: liquid chromatograph, Si: syringe, Vi: three way commutation valve, A: air, CS: conditioning solvent, C: carrier solution, Dil: diluent, W: waste, CC: central channel, EL: eluent, B: channel for bead discarding, Sa: sample/standard solution, HC: holding coil, P: chromatographic pump, IV: injection valve, MC: chromatographic column, λ : diode array detector. Reproduced with kind permission from Springer Science+Business Media.

However, reliable manipulation of bead suspensions within the flow manifold is the major challenge in mechanized BI protocols for repeatable trapping of beads in microcolumns with subsequent minimization of the uncertainty measurement of the overall analytical method. Initially, spherical shape, uniform size distribution and water-wettability (for reversed-phase materials) were identified as imperative requisites for sorbent selection. Recently, novel strategies for microfluidic handling the sorbent suspensions have been proposed (Oliveira et al., 2011), extending the application of LOV-BI to a larger scope of sorbents, not fitting the previous requirements and opening up new opportunities for preconcentration using molecular imprinted polymers for pharmaceutical residue analysis, for instance.

The hyphenation of LOV-BI-MSFIA to chromatography provided a step further on automation for environmental analysis as sample preparation and analyte separation by chromatography were integrated. Previous automation of sample treatment prior to chromatographic analysis involved robotic analyzers, meaning high equipment costs and expensive operation. By using LOV-BI-MSFIA, while one sample is injected in the chromatographic equipment, the following sample is processed in the MSFIA equipment for matrix removal and analyte enrichment. This is an important, advantageous aspect when dealing with labile analytes that cannot sit on automatic injectors for a long time.

As depicted in Fig. 2, connecting the liquid chromatograph equipment to LOV-BI-MSFIA is rather simple requiring that one of the lateral ports of the LOV platform is directly connected to the injection valve present in the chromatograph, allowing the introduction into the injection loop of all eluate or merely a fraction of it via heart-cut injection protocols. The transfer of the entire volume of eluate into the separation system is essential to reach low limits of detection required by analysis of pollutants in environmental samples, especially when using low-sensitivity detectors, for instance UV spectrophotometers. This approach, along with the handling of a well-defined volume of sample (about 10 ml), fostered the determination of non-steroidal anti-inflammatory drugs (NSAIDs) (Quintana et al., 2006) and chlorotriazine herbicides and some of its metabolites (Boonjob et al., 2010) in environmental samples at the low- $\mu\text{g l}^{-1}$ level (Table 3). The screening of UV filters in swimming pool and seawaters also profited from the combination LOV-BI-MSFIA (Oliveira et al., 2010). In-line dilution was necessary after analyte elution in order to match the eluate composition to the aqueous content of the mobile phase, avoiding band broadening problems.

Analyzed species	Working range	Limit of detection	Precision (RSD%)	Reference
Chlorotriazine herbicides	0.1 - 10 $\mu\text{g l}^{-1}$	0.02 - 0.04 $\mu\text{g l}^{-1}$	<5.5	(Boonjob et al., 2010)
Pharmaceutical residues (NSAIDs)	0.4 - 40 $\mu\text{g l}^{-1}$	0.02 - 0.67 $\mu\text{g l}^{-1}$	<11	(Quintana et al., 2006)
Polychlorinated biphenyls	2 - 100 ng l^{-1}	0.5 - 6.1 ng l^{-1}	<9	(Quintana et al., 2009)
UV filters	5 - 160 $\mu\text{g l}^{-1}$	0.45 - 3.2 $\mu\text{g l}^{-1}$	<13	(Oliveira et al., 2010)

Table 3. Analytical figures of LOV-BI-MSFIA system coupled to chromatographic separation

The hyphenation of LOV-BI-MSFIA to gas chromatography is not as simple as it is for liquid chromatography. First, lower injection volumes are required and the analytes should be eluted in a solvent prone to fast vaporization. In fact, only one application has been described so far, where low values for limit of detection were attained through the automatic, on-line transfer of all eluate to a gas chromatograph equipped with an electron capture detector and a programmable temperature vaporization injector for determination of polychlorinated biphenyls in solid-waste leachates at the 2–100 ng L⁻¹ range (Quintana et al, 2009).

4. Conclusions

MSFIA is undoubtedly a suitable automation tool for implementation of environmental analysis. Considering the examples presented here, the proof of concept has been given, shown by application to a large suite of species, comprehending nutrients and pollutants in several environmental matrices. The determination throughputs attained are suitable for most applications sought in environmental monitoring schemes and field deployment is possible for many of the MSFIA systems developed, as long as periodic reagent refilling is guaranteed.

Automation and integration of sample treatment to instrumental quantification of analytes was successfully demonstrated, profiting from the multichannel operation of MSFIA equipment. However, some unique features provided by MSFIA are underexploited for environmental analysis. Recent work regarding LOV-BI-MSFIA coupled to chromatography are still in its infancy and will certainly grow into more reliable, comprehensive analyzers for monitoring of emerging pollutants.

5. Acknowledgement

Financial support from Fundação para a Ciência e Tecnologia (FCT) through grant no. PEst-C/EQB/LA0006/2011 and by European Union through FEDER and QREN 2007-2013 programs (project PTDC/AAC-AMB/104882/2008) is acknowledged. H.M. Oliveira also thanks post-doctoral grant SFRH/BPD/75065/2010.

6. References

- Almeida, M.I.G.S.; Estela, J.M. & Cerdà, V. (2011). Multisyringe Flow Injection Potentialities for Hyphenation with Different Types of Separation Techniques. *Analytical Letters*, Vol.44, No.1-3, (Feb 2011), pp. 360-373, ISSN 0003-2719
- Almeida, M.I.G.S.; Segundo, M.A.; Lima, J.L.F.C. & Rangel, A.O.S.S. (2004). Multi-Syringe Flow Injection System with in-Line Microwave Digestion for the Determination of Phosphorus. *Talanta*, Vol.64, No.5, (Dec 2004), pp. 1283-1289, ISSN 0039-9140
- Almeida, M.I.G.S.; Segundo, M.A.; Lima, J.L.F.C. & Rangel, A.O.S.S. (2005). Multi-Syringe Flow Injection System for the Determination of Available Phosphorus in Soil Samples. *International Journal of Environmental Analytical Chemistry*, Vol.85, No.1, (Jan 2005), pp. 51-62, ISSN 0306-7319

- Almeida, M.I.G.S.; Segundo, M.A.; Lima, J.L.F.C. & Rangel, A.O.S.S. (2006). Potentiometric Multi-Syringe Flow Injection System for Determination of Exchangeable Potassium in Soils with in-Line Extraction. *Microchemical Journal*, Vol.83, No.2, (Jul 2006), pp. 75-80, ISSN 0026-265X
- Almeida, M.I.G.S.; Segundo, M.A.; Lima, J.L.F.C. & Rangel, A.O.S.S. (2008). Direct Introduction of Slurry Samples in Multi-Syringe Flow Injection Analysis: Determination of Potassium in Plant Samples. *Analytical Sciences*, Vol.24, No.5, (May 2008), pp. 601-606, ISSN 0910-6340
- Boonjob, W.; Miró, M. & Cerdà, V. (2008). Multiple Stirred-Flow Chamber Assembly for Simultaneous Automatic Fractionation of Trace Elements in Fly Ash Samples Using a Multisyringe-Based Flow System. *Analytical Chemistry*, Vol.80, No.19, (Oct 2008), pp. 7319-7326, ISSN 0003-2700
- Boonjob, W.; Miró, M.; Segundo, M.A. & Cerdà, V. (2011). Flow-through Dispersed Carbon Nanofiber-Based Microsolid-Phase Extraction Coupled to Liquid Chromatography for Automatic Determination of Trace Levels of Priority Environmental Pollutants. *Analytical Chemistry*, Vol.83, No.13, (Jul 2011), pp. 5237-5244, ISSN 0003-2700
- Boonjob, W.; Yu, Y.L.; Miró, M.; Segundo, M.A.; Wang, J.H. & Cerdà, V. (2010). Online Hyphenation of Multimodal Microsolid Phase Extraction Involving Renewable Molecularly Imprinted and Reversed-Phase Sorbents to Liquid Chromatography for Automatic Multiresidue Assays. *Analytical Chemistry*, Vol.82, No.7, (Apr 2010), pp. 3052-3060, ISSN 0003-2700
- Buanuam, J.; Miró, M.; Hansen, E.H.; Shiohatana, J.; Estela, J.M. & Cerdà, V. (2007). A Multisyringe Flow-through Sequential Extraction System for on-Line Monitoring of Orthophosphate in Soils and Sediments. *Talanta*, Vol.71, No.4, (Mar 2007), pp. 1710-1719, ISSN 0039-9140
- Cerdà, V.; Estela, J.M.; Forteza, R.; Cladera, A.; Becerra, E.; Altimira, P. & Sitjar, P. (1999). Flow Techniques in Water Analysis. *Talanta*, Vol.50, No.4, (Nov 1999), pp. 695-705, ISSN 0039-9140
- Chomchoei, R.; Hansen, E.H. & Shiohatana, J. (2004). Utilizing a Sequential Injection System Furnished with an Extraction Microcolumn as a Novel Approach for Executing Sequential Extractions of Metal Species in Solid Samples. *Analytica Chimica Acta*, Vol.526, No.2, (Nov 2004), pp. 177-184, ISSN 0003-2670
- de Armas, G.; Ferrer, L.; Miró, M.; Estela, J.M. & Cerdà, V. (2004). In-Line Membrane Separation Method for Sulfide Monitoring in Wastewaters Exploiting Multisyringe Flow Injection Analysis. *Analytica Chimica Acta*, Vol.524, No.1-2, (Oct 2004), pp. 89-96, ISSN 0003-2670
- de Armas, G.; Miró, M.; Estela, J.M. & Cerdà, V. (2002). Multisyringe Flow Injection Spectrofluorimetric Determination of Warfarin at Trace Levels with on-Line Solid-Phase Preconcentration. *Analytica Chimica Acta*, Vol.467, No.1-2, (Sep 2002), pp. 13-23, ISSN 0003-2670
- Fernandez, C.; Larrechi, M.S.; Forteza, R.; Cerdà, V. & Callao, M.P. (2010). Multisyringe Chromatography (MSC) Using a Monolithic Column for the Determination of

- Sulphonated Azo Dyes. *Talanta*, Vol.82, No.1, (Jun 2010), pp. 137-142, ISSN 0039-9140
- Ferrer, L.; de Armas, G.; Miró, M.; Estela, J.M. & Cerdà, V. (2004). A Multisyringe Flow Injection Method for the Automated Determination of Sulfide in Waters Using a Miniaturised Optical Fiber Spectrophotometer. *Talanta*, Vol.64, No.5, (Dec 2004), pp. 1119-1126, ISSN 0039-9140
- Ferrer, L.; de Armas, G.; Miró, M.; Estela, J.M. & Cerdà, V. (2005a). Flow-through Optical Fiber Sensor for Automatic Sulfide Determination in Waters by Multisyringe Flow Injection Analysis Using Solid-Phase Reflectometry. *Analyst*, Vol.130, No.5, (May 2005), pp. 644-651, ISSN 0003-2654
- Ferrer, L.; de Armas, G.; Miró, M.; Estela, J.M. & Cerdà, V. (2005b). Interfacing in-Line Gas-Diffusion Separation with Optrode Sorptive Preconcentration Exploiting Multisyringe Flow Injection Analysis. *Talanta*, Vol.68, No.2, (Dec 2005), pp. 343-350, ISSN 0039-9140
- Ferrer, L.; Estela, J.M. & Cerdà, V. (2006). A Smart Multisyringe Flow Injection System for Analysis of Sample Batches with High Variability in Sulfide Concentration. *Analytica Chimica Acta*, Vol.573, (Jul 2006), pp. 391-398, ISSN 0003-2670
- Gomes, D.M.C.; Segundo, M.A.; Lima, J.L.F.C. & Rangel, A.O.S.S. (2005). Spectrophotometric Determination of Iron and Boron in Soil Extracts Using a Multi-Syringe Flow Injection System. *Talanta*, Vol.66, No.3, (Apr 2005), pp. 703-711, ISSN 0039-9140
- Gutzman, Y.; Carroll, A.D. & Ruzicka, J. (2006). Bead Injection for Biomolecular Assays: Affinity Chromatography Enhanced by Bead Injection Spectroscopy. *Analyst*, Vol.131, No.7, (Jul 2006), pp. 809-815, ISSN 0003-2654
- Guzmán-Mar, J.L.; Martínez, L.L.; de Alba, P.L.L.; Duran, J.E.C. & Martín, V.C. (2006a). Multisyringe Flow Injection Analysis for Determination of 1-Naphthylamine in Water Samples. *Microchimica Acta*, Vol.153, No.3-4, (Feb 2006), pp. 139-144, ISSN 0026-3672
- Guzmán-Mar, J.L.; Martínez, L.L.; de Alba, P.L.L.; Duran, J.E.C. & Martín, V.C. (2006b). Optical Fiber Reflectance Sensor Coupled to a Multisyringe Flow Injection System for Preconcentration and Determination of 1-Naphthylamine in Water Samples. *Analytica Chimica Acta*, Vol.573, (Jul 2006), pp. 406-412, ISSN 0003-2670
- Horstkotte, B.; Elsholz, O. & Martín, V.C. (2008). Multisyringe Flow Injection Analysis Coupled to Capillary Electrophoresis (MSFIA-CE) as a Novel Analytical Tool Applied to the Pre-Concentration, Separation and Determination of Nitrophenols. *Talanta*, Vol.76, No.1, (Jun 2008), pp. 72-79, ISSN 0039-9140
- Leal, L.O.; Elsholz, O.; Forteza, R. & Cerdà, V. (2006a). Determination of Mercury by Multisyringe Flow Injection System with Cold-Vapor Atomic Absorption Spectrometry. *Analytica Chimica Acta*, Vol.573, (Jul 2006), pp. 399-405, ISSN 0003-2670

- Leal, L.O.; Forteza, R. & Cerdà, V. (2006b). Speciation Analysis of Inorganic Arsenic by a Multisyringe Flow Injection System with Hydride Generation-Atomic Fluorescence Spectrometric Detection. *Talanta*, Vol.69, No.2, (Apr 2006), pp. 500-508, ISSN 0039-9140
- Long, X.B.; Miró, M.; Hansen, E.H.; Estela, J.M. & Cerdà, V. (2006). Hyphenating Multisyringe Flow Injection Lab-on-Valve Analysis with Atomic Fluorescence Spectrometry for on-Line Bead Injection Preconcentration and Determination of Trace Levels of Hydride-Forming Elements in Environmental Samples. *Analytical Chemistry*, Vol.78, No.24, (Dec 2006), pp. 8290-8298, ISSN 0003-2700
- Magalhães, L.M.; Ribeiro, J.P.N.; Segundo, M.A.; Reis, S. & Lima, J.L.F.C. (2009). Multi-Syringe Flow-Injection Systems Improve Antioxidant Assessment. *Trac-Trends in Analytical Chemistry*, Vol.28, No.8, (Sep 2009), pp. 952-960, ISSN 0165-9936
- Manera, M.; Miró, M.; Estela, J.M. & Cerdà, V. (2007a). Multi-Syringe Flow Injection Solid-Phase Extraction System for on-Line Simultaneous Spectrophotometric Determination of Nitro-Substituted Phenol Isomers. *Analytica Chimica Acta*, Vol.582, No.1, (Jan 2007), pp. 41-49, ISSN 0003-2670
- Manera, M.; Miró, M.; Estela, J.M.; Cerdà, V.; Segundo, M.A. & Lima, J.L.F.C. (2007b). Flow-through Solid-Phase Reflectometric Method for Simultaneous Multiresidue Determination of Nitrophenol Derivatives. *Analytica Chimica Acta*, Vol.600, No.1-2, (Sep 2007), pp. 155-163, ISSN 0003-2670
- Maya, F.; Estela, J.M. & Cerdà, V. (2007). Improving the Chemiluminescence-Based Determination of Sulphide in Complex Environmental Samples by Using a New, Automated Multi-Syringe Flow Injection Analysis System Coupled to a Gas Diffusion Unit. *Analytica Chimica Acta*, Vol.601, No.1, (Oct 2007), pp. 87-94, ISSN 0003-2670
- Maya, F.; Estela, J.M. & Cerdà, V. (2008). Completely Automated System for Determining Halogenated Organic Compounds by Multisyringe Flow Injection Analysis. *Analytical Chemistry*, Vol.80, No.15, (Aug 2008), pp. 5799-5805, ISSN 0003-2700
- Maya, F.; Estela, J.M. & Cerdà, V. (2009). Multisyringe Flow Injection Technique for Development of Green Spectroscopic Analytical Methodologies. *Spectroscopy Letters*, Vol.42, No.6-7, (Dec 2009), pp. 312-319, ISSN 0038-7010
- Maya, F.; Estela, J.M. & Cerdà, V. (2010). Interfacing on-Line Solid Phase Extraction with Monolithic Column Multisyringe Chromatography and Chemiluminescence Detection: An Effective Tool for Fast, Sensitive and Selective Determination of Thiazide Diuretics. *Talanta*, Vol.80, No.3, (Jan 2010), pp. 1333-1340, ISSN 0039-9140
- Miró, M.; Cerdà, V. & Estela, J.M. (2002). Multisyringe Flow Injection Analysis: Characterization and Applications. *Trac-Trends in Analytical Chemistry*, Vol.21, No.3, (Mar 2002), pp. 199-210, ISSN 0165-9936
- Miró, M.; Cladera, A.; Estela, J.M. & Cerdà, V. (2001). Dual Wetting-Film Multi-Syringe Flow Injection Analysis Extraction - Application to the Simultaneous Determination of

- Nitrophenols. *Analytica Chimica Acta*, Vol.438, No.1-2, (Jul 2001), pp. 103-116, ISSN 0003-2670
- Miró, M.; Oliveira, H.M. & Segundo, M.A. (2011). Analytical Potential of Mesofluidic Lab-on-a-Valve as a Front End to Column-Separation Systems. *Trac-Trends in Analytical Chemistry*, Vol.30, No.1, (Jan 2011), pp. 153-164, ISSN 0165-9936
- Morais, I.P.A.; Miró, M.; Manera, M.; Estela, J.M.; Cerdà, V.; Souto, M.R.S. & Rangel, A.O.S.S. (2004). Flow-through Solid-Phase Based Optical Sensor for the Multisyringe Flow Injection Trace Determination of Orthophosphate in Waters with Chemiluminescence Detection. *Analytica Chimica Acta*, Vol.506, No.1, (Mar 2004), pp. 17-24, ISSN 0003-2670
- Oliveira, H.M.; Miró, M.; Segundo, M.A. & Lima, J.L.F.C. (2011). Universal Approach for Mesofluidic Handling of Bead Suspensions in Lab-on-Valve Format. *Talanta*, Vol.84, No.3, (May 2011), pp. 846-852, ISSN 0039-9140
- Oliveira, H.M.; Segundo, M.A.; Lima, J.L.F.C. & Cerdà, V. (2009). Multisyringe Flow Injection System for Solid-Phase Extraction Coupled to Liquid Chromatography Using Monolithic Column for Screening of Phenolic Pollutants. *Talanta*, Vol.77, No.4, (Feb 2009), pp. 1466-1472, ISSN 0039-9140
- Oliveira, H.M.; Segundo, M.A.; Lima, J.L.F.C.; Miró, M. & Cerdà, V. (2010). On-Line Renewable Solid-Phase Extraction Hyphenated to Liquid Chromatography for the Determination of UV Filters Using Bead Injection and Multisyringe-Lab-on-Valve Approach. *Journal of Chromatography A*, Vol.1217, No.22, (May 2010), pp. 3575-3582, ISSN 0021-9673
- Oliveira, H.M.; Segundo, M.A.; Reis, S. & Lima, J.L.F.C. (2005). Multi-Syringe Flow Injection System with in-Line Pre-Concentration for the Determination of Total Phenolic Compounds. *Microchimica Acta*, Vol.150, No.2, (Jun 2005), pp. 187-196, ISSN 1436-5073
- Ornelas-Soto, N.E.; Guzman-Mar, J.L.; de Alba, P.L.L.; Martinez, L.L.; Barbosa-Garcia, O. & Martin, V.C. (2009). Coupled Multisyringe Flow Injection/Reactor Tank for the Spectrophotometric Detection of Azinphos Methyl in Water Samples. *Microchimica Acta*, Vol.167, No.3-4, (Dec 2009), pp. 273-280, ISSN 0026-3672
- Pascoa, R.N.M.J.; Toth, I.V. & Rangel, A.O.S.S. (2009). A Multi-Syringe Flow Injection System for the Spectrophotometric Determination of Trace Levels of Iron in Waters Using a Liquid Waveguide Capillary Cell and Different Chelating Resins and Reaction Chemistries. *Microchemical Journal*, Vol.93, No.2, (Nov 2009), pp. 153-158, ISSN 0026-265X
- Pons, C.; Forteza, R. & Cerdà, V. (2004). Expert Multi-Syringe Flow-Injection System for the Determination and Speciation Analysis of Iron Using Chelating Disks in Water Samples. *Analytica Chimica Acta*, Vol.524, No.1-2, (Oct 2004), pp. 79-88, ISSN 0003-2670
- Pons, C.; Forteza, R. & Cerdà, V. (2005a). Optical Fibre Reflectance Sensor for the Determination and Speciation Analysis of Iron in Fresh and Seawater Samples

- Coupled to a Multisyringe Flow Injection System. *Analytica Chimica Acta*, Vol.528, No.2, (Jan 2005), pp. 197-203, ISSN 0003-2670
- Pons, C.; Forteza, R. & Cerdà, V. (2005b). The Use of Anion-Exchange Disks in an Optrode Coupled to a Multi-Syringe Flow-Injection System for the Determination and Speciation Analysis of Iron in Natural Water Samples. *Talanta*, Vol.66, No.1, (Mar 2005), pp. 210-217, ISSN 0039-9140
- Quintana, J.B.; Boonjob, W.; Miró, M. & Cerdà, V. (2009). Online Coupling of Bead Injection Lab-on-Valve Analysis to Gas Chromatography: Application to the Determination of Trace Levels of Polychlorinated Biphenyls in Solid Waste Leachates. *Analytical Chemistry*, Vol.81, No.12, (Jun 2009), pp. 4822-4830, ISSN 0003-2700
- Quintana, J.B.; Miró, M.; Estela, J.M. & Cerdà, V. (2006). Automated on-Line Renewable Solid-Phase Extraction-Liquid Chromatography Exploiting Multisyringe Flow Injection-Bead Injection Lab-on-Valve Analysis. *Analytical Chemistry*, Vol.78, No.8, (Apr 2006), pp. 2832-2840, ISSN 0003-2700
- Rosende, M.; Miró, M.; Segundo, M.A.; Lima, J.L.F.C. & Cerdà, V. (2011). Highly Integrated Flow Assembly for Automated Dynamic Extraction and Determination of Readily Bioaccessible Chromium(VI) in Soils Exploiting Carbon Nanoparticle-Based Solid-Phase Extraction. *Analytical and Bioanalytical Chemistry*, Vol.400, No.7, (Jun 2011), pp. 2217-2227, ISSN 1618-2642
- Ruzicka, J. & Hansen, E.H. (1975). Flow Injection Analyses. 1. New Concept of Fast Continuous-Flow Analysis. *Analytica Chimica Acta*, Vol.78, No.1, (Aug 1975), pp. 145-157, ISSN 0003-2670
- Ruzicka, J. & Marshall, G.D. (1990). Sequential Injection - a New Concept for Chemical Sensors, Process Analysis and Laboratory Assays. *Analytica Chimica Acta*, Vol.237, No.2, (Oct 1990), pp. 329-343, ISSN 0003-2670
- Segundo, M.A. & Magalhães, L.M. (2006). Multisyringe Flow Injection Analysis: State-of-the-Art and Perspectives. *Analytical Sciences*, Vol.22, No.1, (Jan 2006), pp. 3-8, ISSN 0910-6340
- Semenova, N.V.; Leal, L.O.; Forteza, R. & Cerdà, V. (2002). Multisyringe Flow-Injection System for Total Inorganic Arsenic Determination by Hydride Generation-Atomic Fluorescence Spectrometry. *Analytica Chimica Acta*, Vol.455, No.2, (Mar 2002), pp. 277-285, ISSN 0003-2670
- Semenova, N.V.; Leal, L.O.; Forteza, R. & Cerdà, V. (2003). Multisyringe Flow Injection System for Total Inorganic Selenium Determination by Hydride Generation-Atomic Fluorescence Spectrometry. *Analytica Chimica Acta*, Vol.486, No.2, (Jun 2003), pp. 217-225, ISSN 0003-2670
- Serra, A.M.; Estela, J.M. & Cerdà, V. (2008). MSFIA System for Mercury Determination by Cold Vapour Technique with Atomic Fluorescence Detection. *Talanta*, Vol.77, No.2, (Dec 2008), pp. 556-560, ISSN 0039-9140
- Serra, A.M.; Estela, J.M. & Cerdà, V. (2009). An MSFIA System for Mercury Speciation Based on an Anion-Exchange Membrane. *Talanta*, Vol.78, No.3, (May 2009), pp. 790-794, ISSN 0039-9140

Serra, A.M.; Estela, J.M.; Coulomb, B.; Boudenne, J.L. & Cerdà, V. (2010). Solid Phase Extraction - Multisyringe Flow Injection System for the Spectrophotometric Determination of Selenium with 2,3-Diaminonaphthalene. *Talanta*, Vol.81, No.1-2, (Apr 2010), pp. 572-577, ISSN 0039-9140

IntechOpen

IntechOpen



Environmental Monitoring

Edited by Dr Ema Ekundayo

ISBN 978-953-307-724-6

Hard cover, 528 pages

Publisher InTech

Published online 04, November, 2011

Published in print edition November, 2011

"Environmental Monitoring" is a book designed by InTech - Open Access Publisher in collaboration with scientists and researchers from all over the world. The book is designed to present recent research advances and developments in the field of environmental monitoring to a global audience of scientists, researchers, environmental educators, administrators, managers, technicians, students, environmental enthusiasts and the general public. The book consists of a series of sections and chapters addressing topics like the monitoring of heavy metal contaminants in varied environments, biological monitoring/ecotoxicological studies; and the use of wireless sensor networks/Geosensor webs in environmental monitoring.

How to reference

In order to correctly reference this scholarly work, feel free to copy and paste the following:

Marcela A. Segundo, M. Inês G. S. Almeida and Hugo M. Oliveira (2011). Multisyringe Flow Injection Analysis for Environmental Monitoring: Applications and Recent Trends, Environmental Monitoring, Dr Ema Ekundayo (Ed.), ISBN: 978-953-307-724-6, InTech, Available from: <http://www.intechopen.com/books/environmental-monitoring/multisyringe-flow-injection-analysis-for-environmental-monitoring-applications-and-recent-trends>

INTECH

open science | open minds

InTech Europe

University Campus STeP Ri
Slavka Krautzeka 83/A
51000 Rijeka, Croatia
Phone: +385 (51) 770 447
Fax: +385 (51) 686 166
www.intechopen.com

InTech China

Unit 405, Office Block, Hotel Equatorial Shanghai
No.65, Yan An Road (West), Shanghai, 200040, China
中国上海市延安西路65号上海国际贵都大饭店办公楼405单元
Phone: +86-21-62489820
Fax: +86-21-62489821

© 2011 The Author(s). Licensee IntechOpen. This is an open access article distributed under the terms of the [Creative Commons Attribution 3.0 License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

IntechOpen

IntechOpen